


# EU compliance: UDI labelling deadlines for medical devices and IVDs

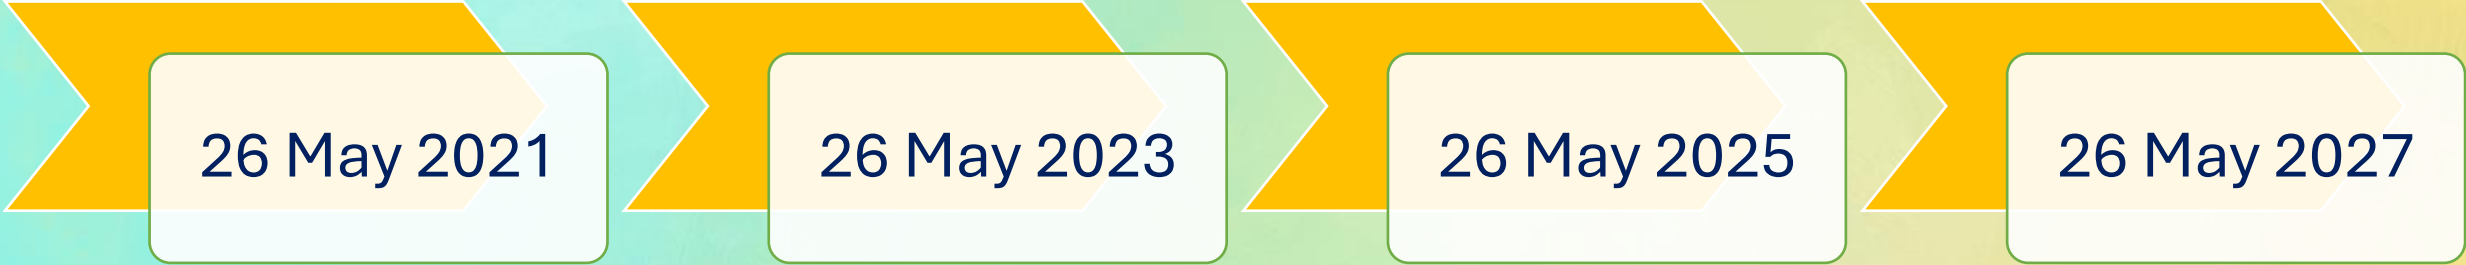

**Implantable devices  
Class III devices**

**Class IIa devices  
Class IIb devices  
Class D IVDs**

**Class I devices  
Class C and B IVDs**

**Class A IVDs**



Data refer to timelines for placing UDI-carriers on the labels of devices. Different deadlines apply for direct marking of reusable devices.